



Microplate, 384-well 781980

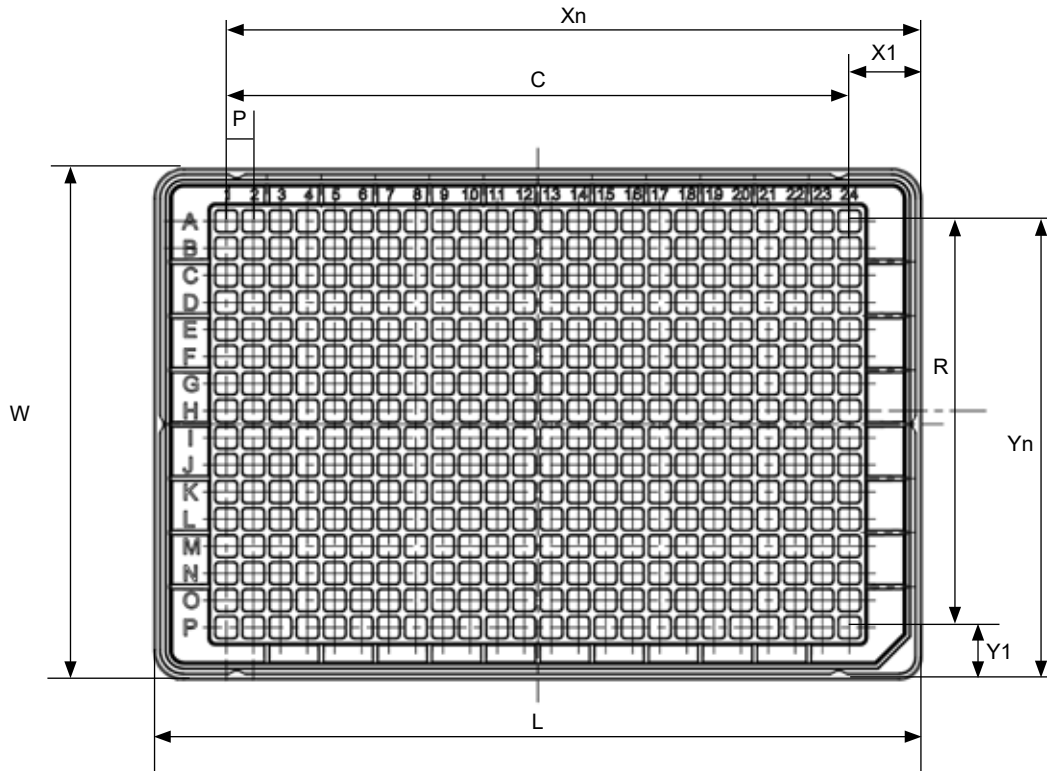

| | |
|----|-----------|
| L | 127.55 mm |
| W | 85.05 mm |
| H | 11.50 mm |
| Hs | 3.50 mm |
| X1 | 12.03 mm |
| Xn | 115.53 mm |
| Y1 | 8.78 mm |
| Yn | 76.28 mm |
| P | 4.50 mm |
| D | 3.90 mm |
| Hw | 8.85 mm |
| C | 24 Well |
| R | 16 Well |

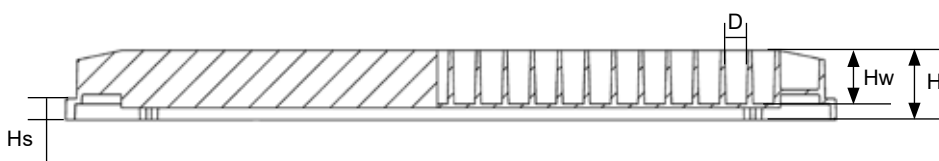


| | |
|------------|---|
| Type | standard |
| Base shape | F-bottom |
| Surface | cellGrade™ |
| Volume | 100 µl / well |
| Material | PS |
| Color | transparent |
| Quality | Cleanroom class 8 according to ISO 14 644-1, Free of DNA*, RNase and DNase, Free of pyrogens, according to LAL test **, Sterile according to ISO 11 137, Free of cytotoxic substances acc. ISO 10 993-5 |




* human and bacterial DNA, ** according to Limulus Amebocyte Lysate (LAL) test, detection limit 0.01 EU/ml

Subject to technical modification without notice. Errors excepted.

Microplate, 96-well 781981

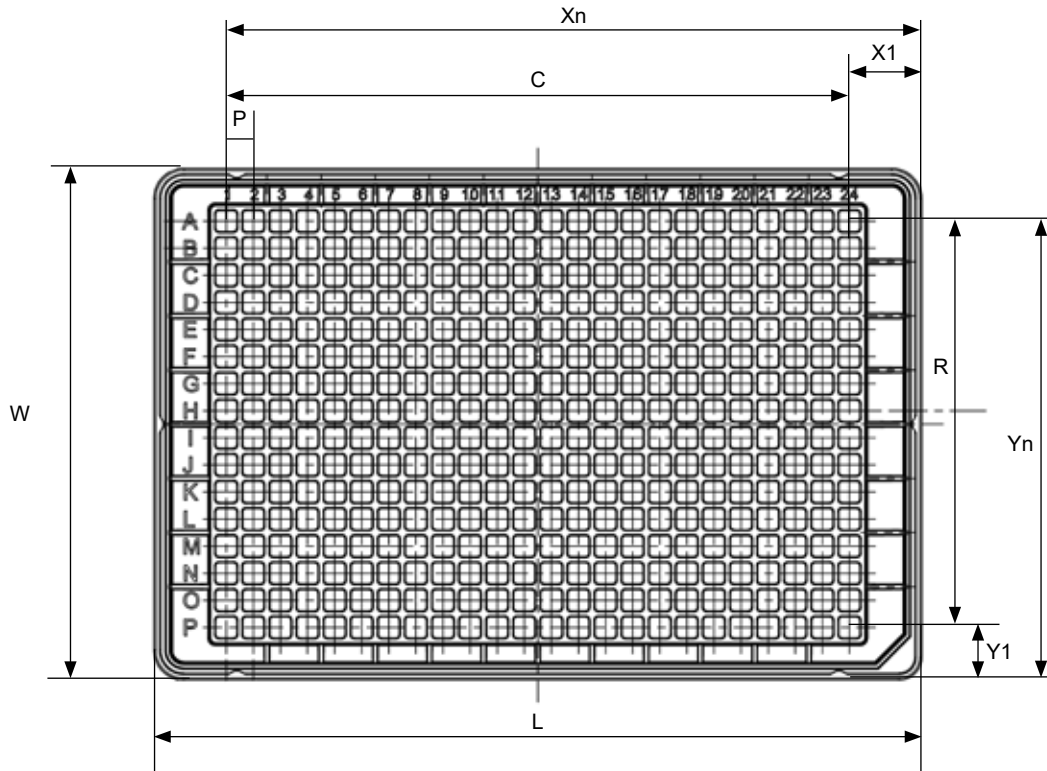

| | |
|----|-----------|
| L | 127.55 mm |
| W | 85.05 mm |
| H | 11.50 mm |
| Hs | 3.50 mm |
| X1 | 12.03 mm |
| Xn | 115.53 mm |
| Y1 | 8.78 mm |
| Yn | 76.28 mm |
| P | 4.50 mm |
| D | 3.90 mm |
| Hw | 8.85 mm |
| C | 24 Well |
| R | 16 Well |

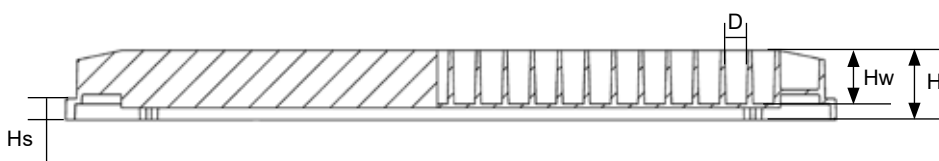


| | |
|------------|---|
| Type | standard |
| Base shape | F-bottom |
| Surface | cellGrade™ |
| Volume | 100 µl / well |
| Material | PS |
| Color | white |
| Quality | Cleanroom class 8 according to ISO 14 644-1, Free of DNA*, RNase and DNase, Free of pyrogens, according to LAL test **, Sterile according to ISO 11 137, Free of cytotoxic substances acc. ISO 10 993-5 |




* human and bacterial DNA, ** according to Limulus Amebocyte Lysate (LAL) test, detection limit 0.01 EU/ml

Subject to technical modification without notice. Errors excepted.

Microplate, 96-well 781982

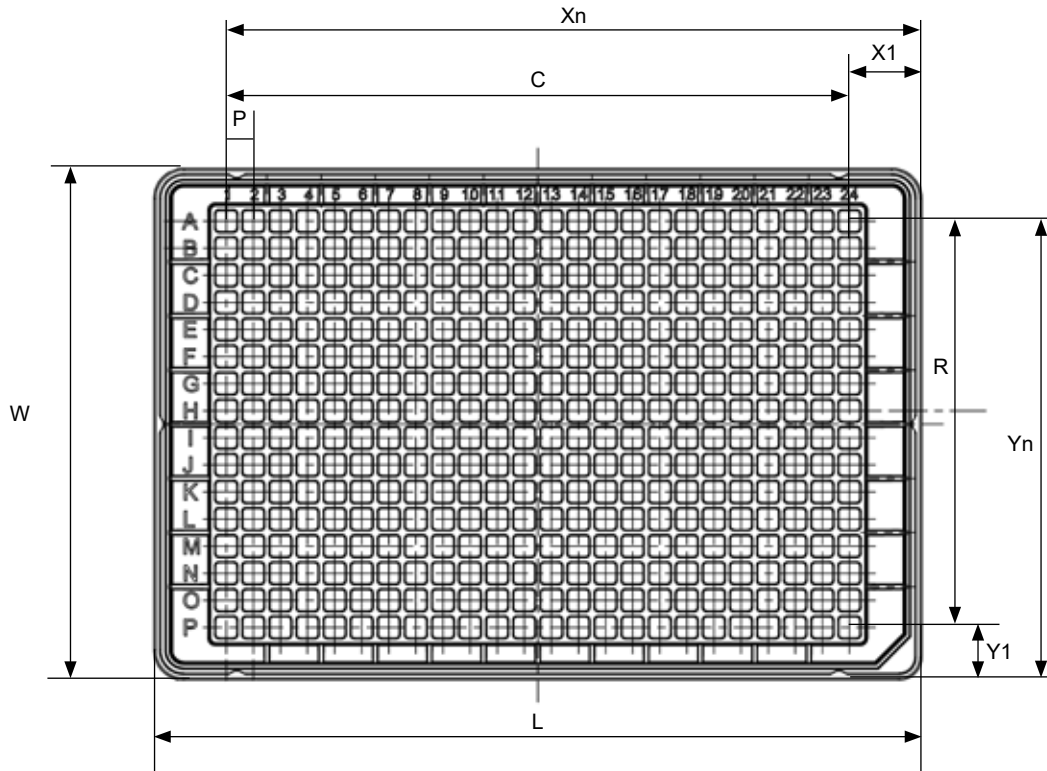

| | |
|----|-----------|
| L | 127.55 mm |
| W | 85.05 mm |
| H | 11.50 mm |
| Hs | 3.50 mm |
| X1 | 12.03 mm |
| Xn | 115.53 mm |
| Y1 | 8.78 mm |
| Yn | 76.28 mm |
| P | 4.50 mm |
| D | 3.90 mm |
| Hw | 8.85 mm |
| C | 24 Well |
| R | 16 Well |

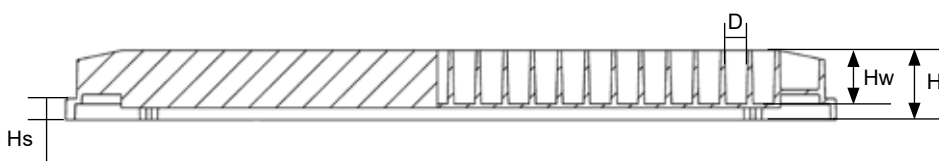


| | |
|------------|---|
| Type | standard |
| Base shape | F-bottom |
| Surface | cellGrade™ |
| Volume | 100 µl / well |
| Material | PS |
| Color | black |
| Quality | Cleanroom class 8 according to ISO 14 644-1, Free of DNA*, RNase and DNase, Free of pyrogens, according to LAL test **, Sterile according to ISO 11 137, Free of cytotoxic substances acc. ISO 10 993-5 |



* human and bacterial DNA, ** according to Limulus Amebocyte Lysate (LAL) test, detection limit 0.01 EU/ml

Subject to technical modification without notice. Errors excepted.

Microplate, 96-well 781986, 781988

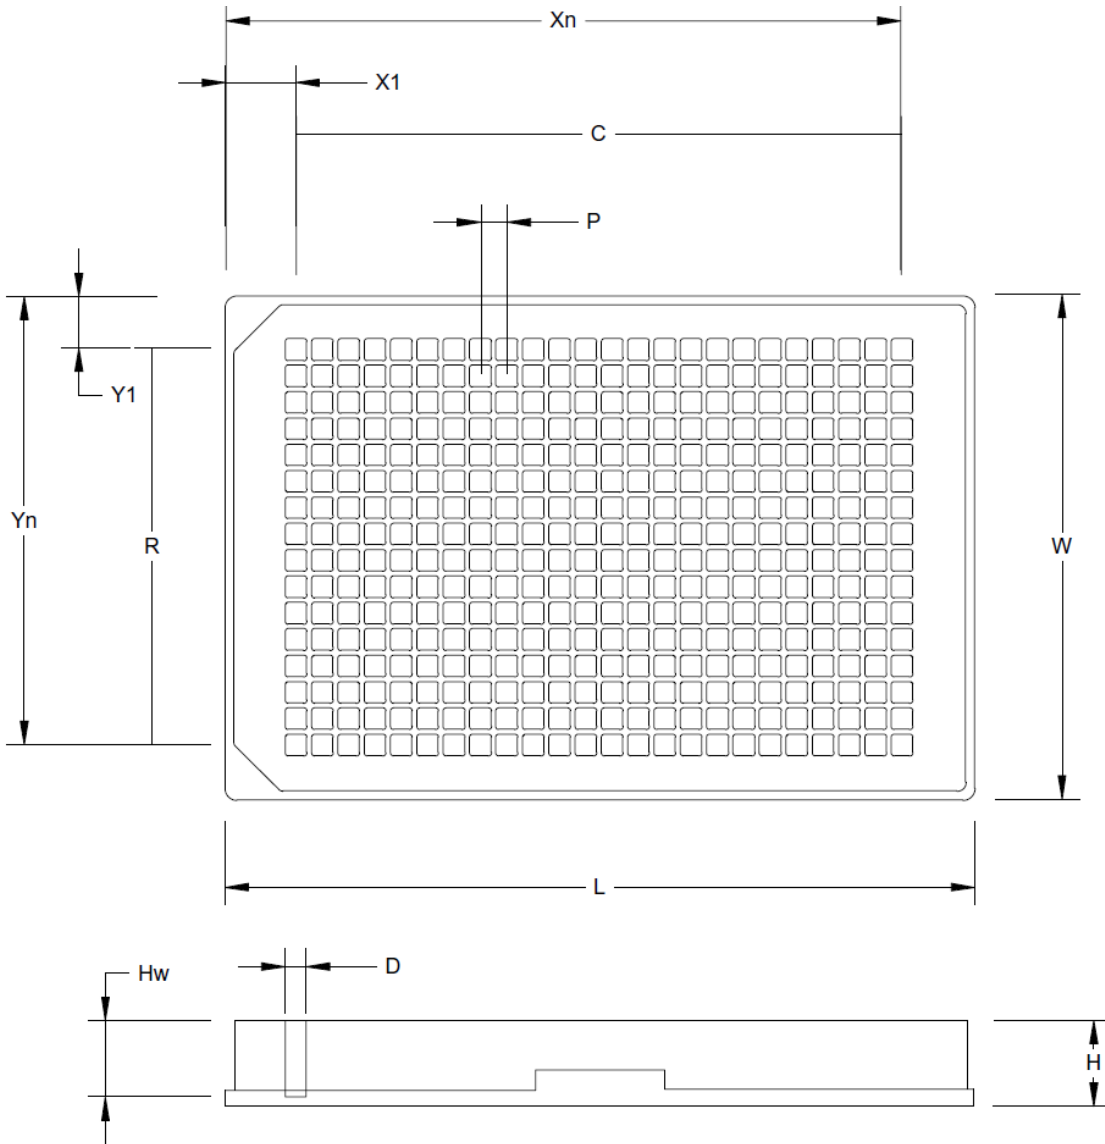

| | |
|----|-----------|
| L | 127.60 mm |
| W | 85.60 mm |
| H | 14.80 mm |
| Hs | 2.75 mm |
| X1 | 12.10 mm |
| Xn | 115.60 mm |
| Y1 | 9.10 mm |
| Yn | 76.60 mm |
| P | 4.50 mm |
| D | 3.65 mm |
| Hw | 11.95 mm |
| C | 24 Well |
| R | 16 Well |

| | |
|------------|---|
| Type | standard, transparent bottom |
| Base shape | F-bottom |
| Surface | cellGrade™ |
| Volume | 120 µl / well |
| Material | PS |
| Color | white |
| Quality | Cleanroom class 8 according to ISO 14 644-1, Free of DNA*, RNase and DNase, Free of pyrogens, according to LAL test **, Sterile according to ISO 11 137, Free of cytotoxic substances acc. ISO 10 993-5 |




* human and bacterial DNA, ** according to Limulus Amebocyte Lysate (LAL) test, detection limit 0.01 EU/ml

Subject to technical modification without notice. Errors excepted.

Microplate, 96-well

781987, 781989

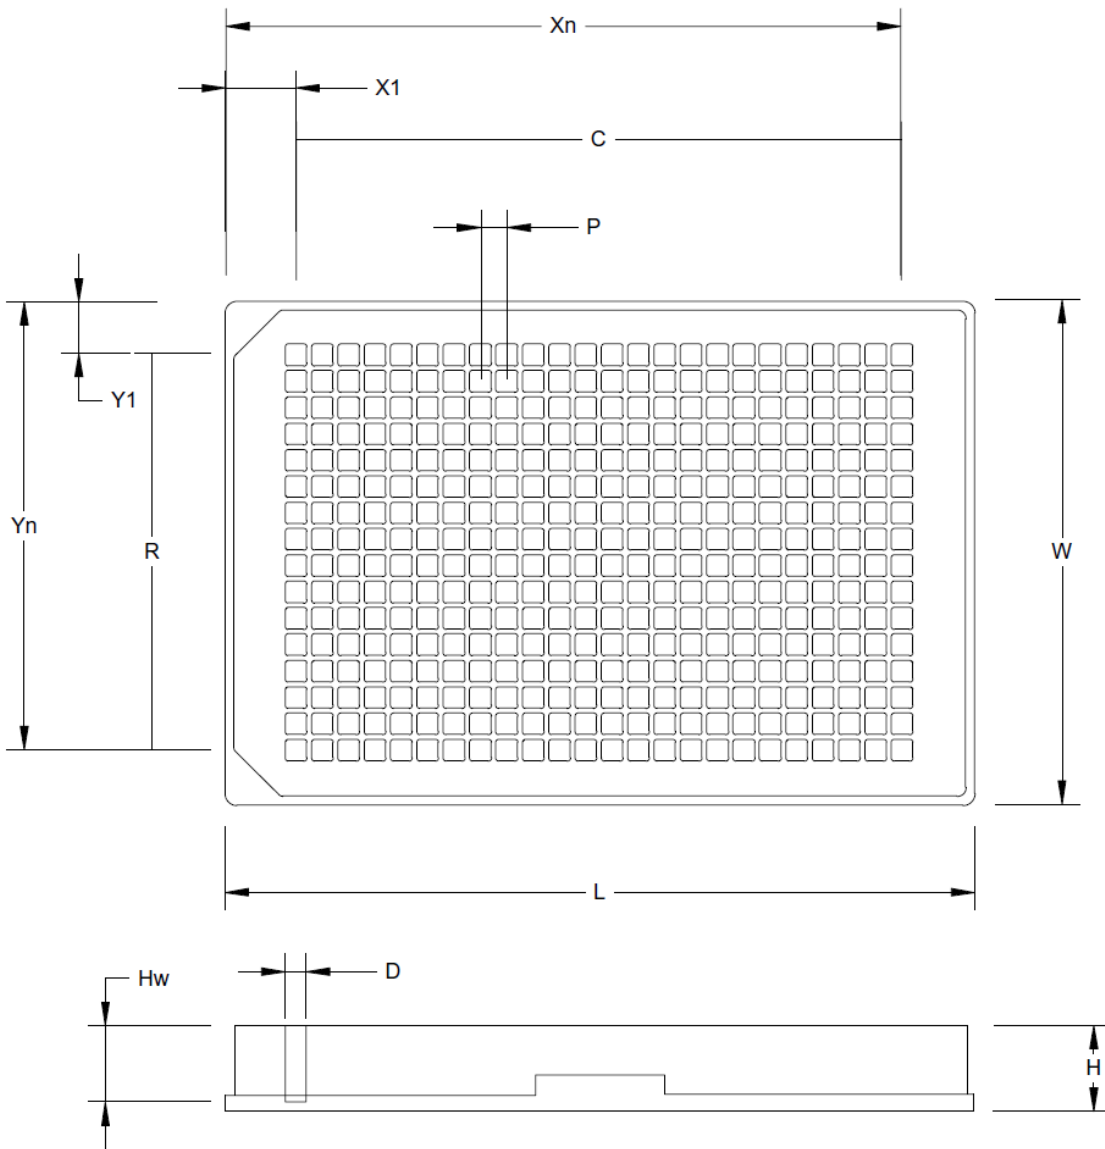

| | |
|----|-----------|
| L | 127.60 mm |
| W | 85.60 mm |
| H | 14.80 mm |
| Hs | 2.75 mm |
| X1 | 12.10 mm |
| Xn | 115.60 mm |
| Y1 | 9.10 mm |
| Yn | 76.60 mm |
| P | 4.50 mm |
| D | 3.65 mm |
| Hw | 11.95 mm |
| C | 24 Well |
| R | 16 Well |

| | |
|------------|---|
| Type | standard, transparent bottom |
| Base shape | F-bottom |
| Surface | cellGrade™ |
| Volume | 120 µl / well |
| Material | PS |
| Color | black |
| Quality | Cleanroom class 8 according to ISO 14 644-1, Free of DNA*, RNase and DNase, Free of pyrogens, according to LAL test **, Sterile according to ISO 11 137, Free of cytotoxic substances acc. ISO 10 993-5 |



* human and bacterial DNA, ** according to Limulus Amebocyte Lysate (LAL) test, detection limit 0.01 EU/ml

Subject to technical modification without notice. Errors excepted.